



Electrical

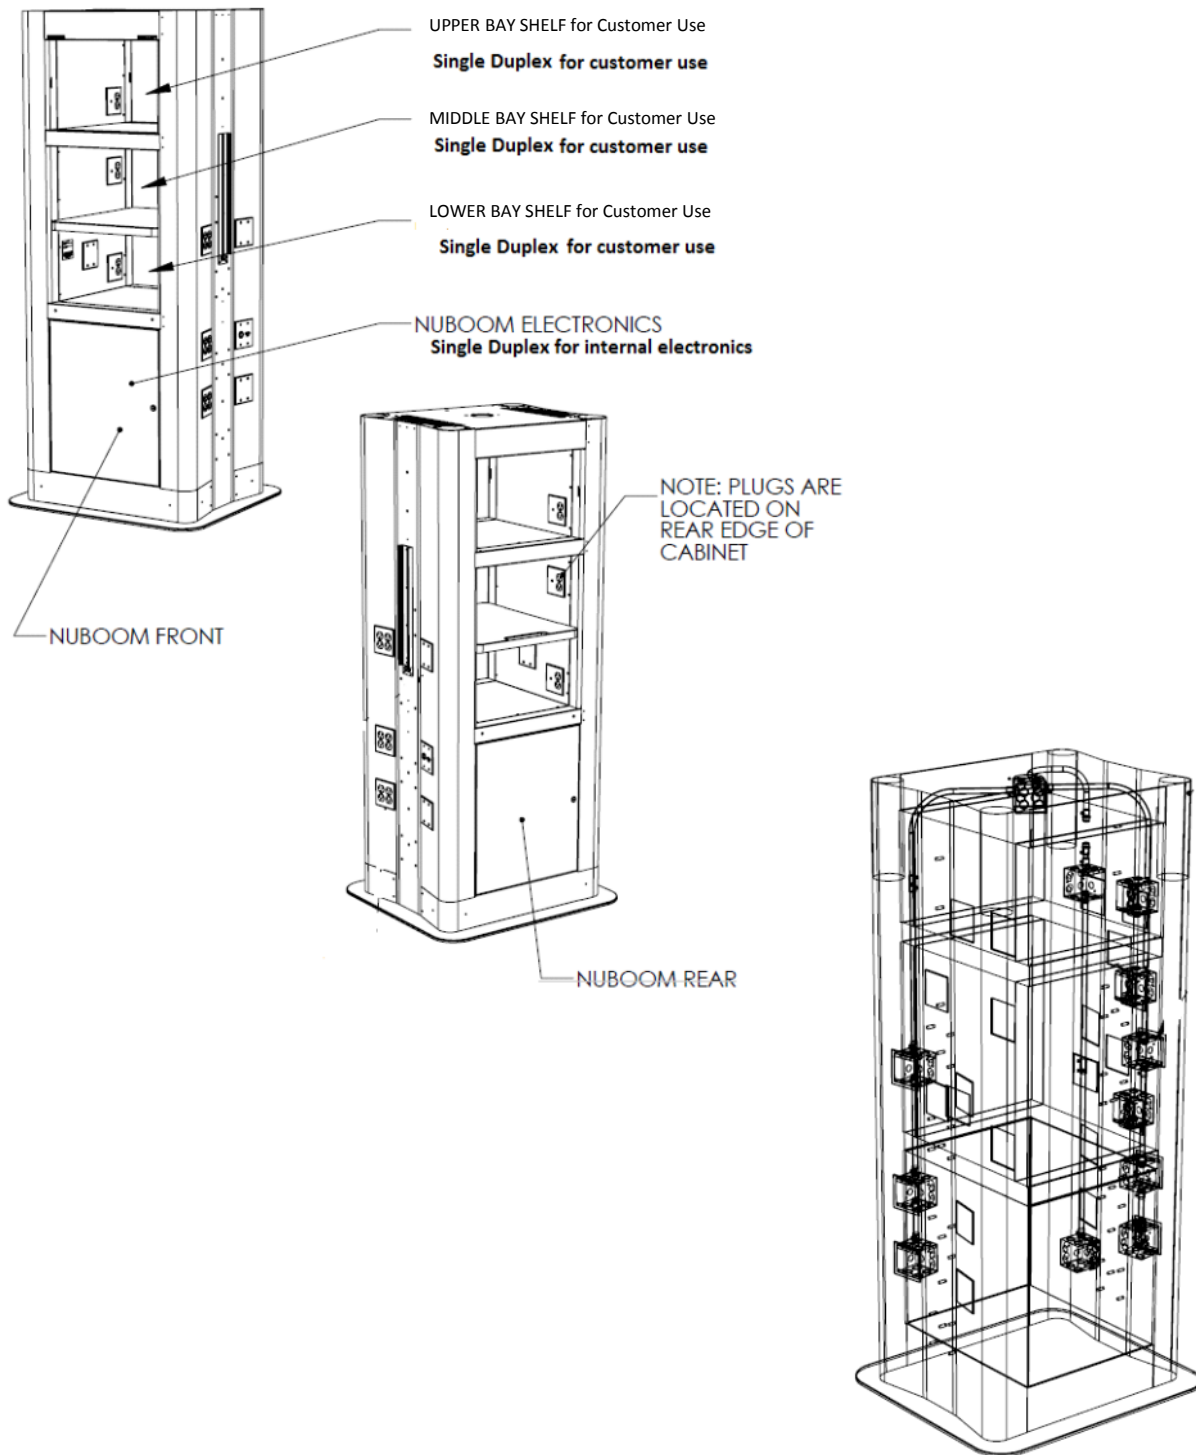

Critical Power Circuits 120 x 20 each

Number of Receptacles available for Customer use is dependent upon Local Electrical Code Allowance per Circuit and Load of Accessory Equipment.

J-Boxes highlighted are the minimum receptacles recommended for standard accessory equipment usage.

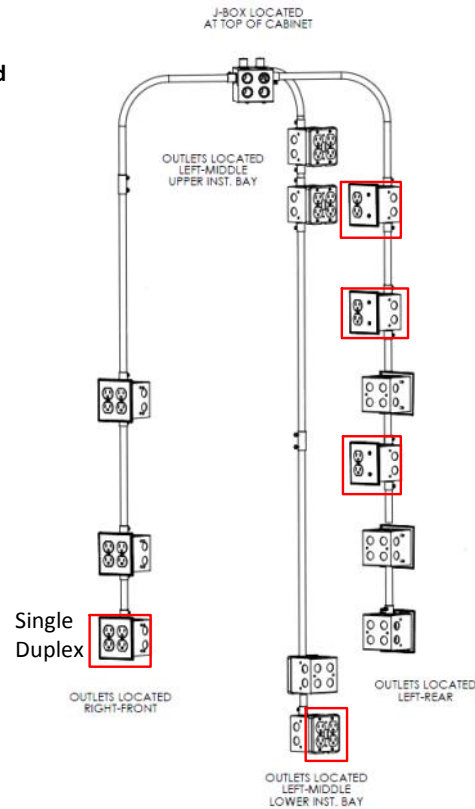

Three Raceways Pre-installed:

Right Front: 1 duplex

*(possibly: table, warmer or c-arm)

Left Middle: Dedicated Circuit & 1 duplex for Internal Use Only
(electronic rack, monitors)

Left Rear: 3 Duplex Receptacles

*(one per bay shelf for Accessory Equipment)

- Dependent upon the Facility's desired Accessory Equipment to be energized by the Nuboom cabinet, some may require a Dedicated Circuit due to device electrical load requirements.
- Accessory Equipment may include but not limited to:
scope, light source, recording device, procedure table, c-arm, warming unit, cautery, laser
- Wiring of cabinet and overhead connection is the responsibility of the Customer.