


EQUIPMENT DETAIL
REVOLUTION XQ/i TUBESTAND

B35-25
REV. DATE: 05/17/05


SHIPPING DIMENSIONS:
96"(2440mm)L x 37"(940mm)W x 40"(1020mm)H

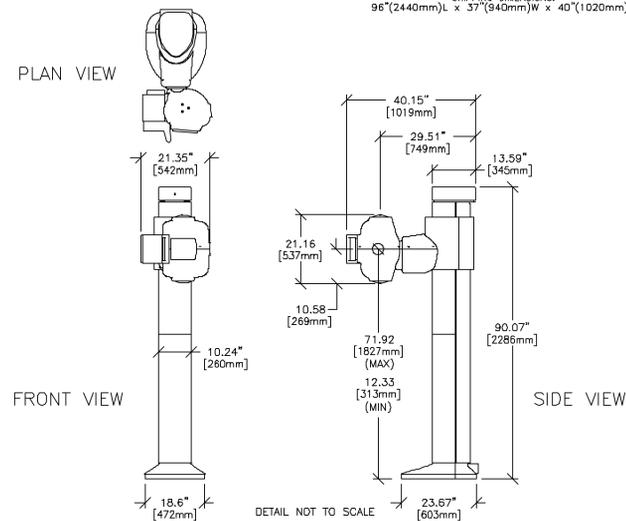

EQUIPMENT DETAIL
REVOLUTION XQ/i DIGITAL CHEST READER


B35-25D
REV. DATE: 05/17/05

SHIPPING DIMENSIONS:
96"(2440mm)L x 37"(940mm)W x 40"(1020mm)H

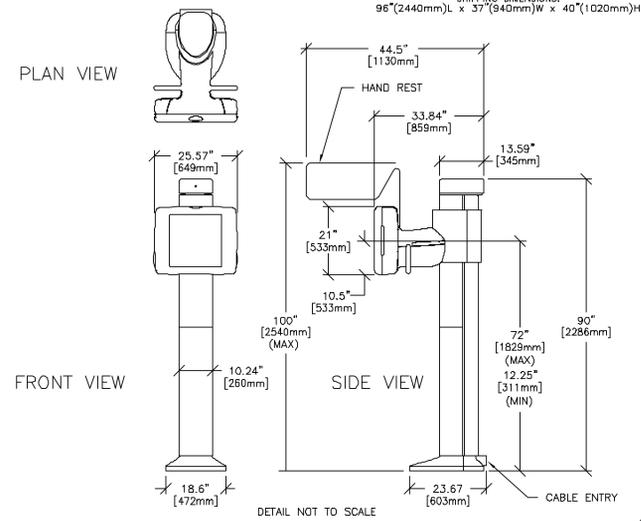


EQUIPMENT DETAIL
CONTROL CONSOLE

A80066
REV. DATE: 03/10/99

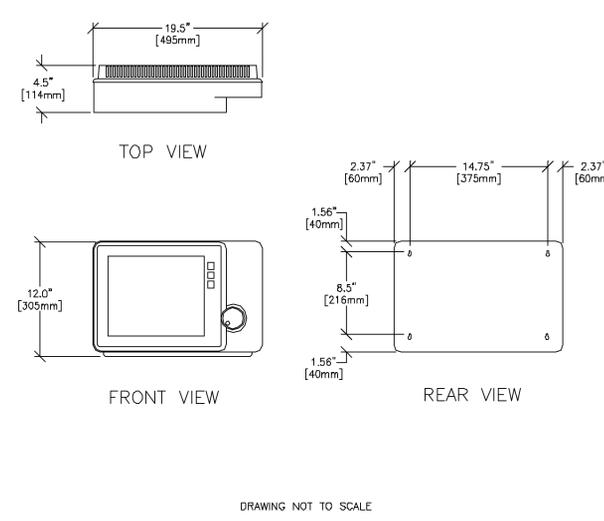

EQUIPMENT DETAIL
REVOLUTION ACQUISITION DIGITAL STATION


B35-25C
REV. DATE: 10/30/01

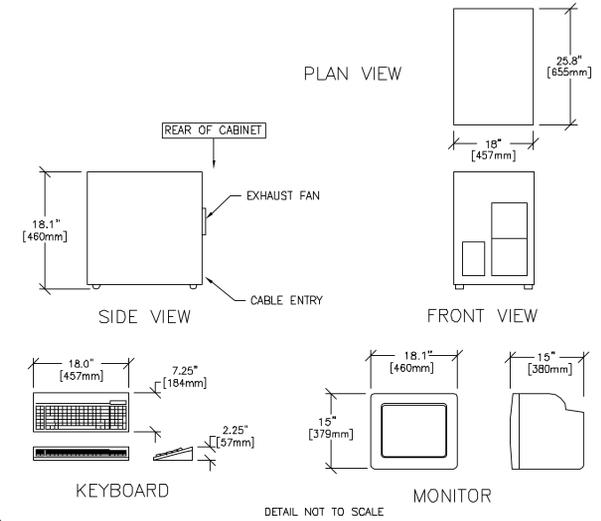

EQUIPMENT DETAIL
REVOLUTION GENERATOR

A07-20B
REV. DATE: 05/17/05


SHIPPING DIMENSIONS:
24.8"(630mm)L x 50"(1270mm)W x 82.3"(2090mm)H

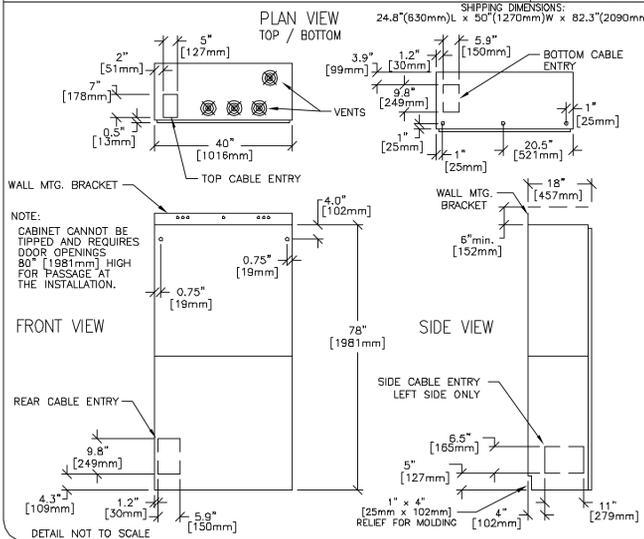

EQUIPMENT DETAIL
DETECTOR SUPPORT ASSEMBLY

B05-57D
REV. DATE: 05/17/05

SHIPPING DIMENSIONS:
24"(610mm)L x 18"(457mm)W x 24"(610mm)H

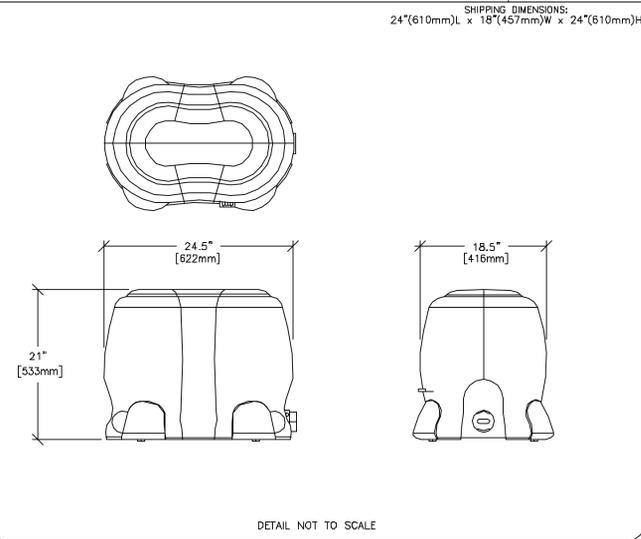

This drawing is based on Sketch No.: 111mcc047 VA Brooklyn QXi revision

PIM R3

RQ - 119540

SHEET TITLE: EQUIPMENT DETAILS
MODALITY TYPE: REVOLUTION XQ/i

PROJECT TITLE:
VA BROOKLYN
MEDICAL CENTER
BROOKLYN, NEW YORK

| PROJECT | REVISION |
|-------------|-----------|
| 111639 | 00 |
| DATE: | 01.Jul.11 |
| DRAWN BY: | CPC |
| CHECKED BY: | REK |

REVISION HISTORY:

SHEET
D1

THIS PLAN IS SUBMITTED TO SUGGEST LOCATION OF GE HEALTHCARE EQUIPMENT. GE HEALTHCARE EQUIPMENT IS NOT TO BE INSTALLED. IT IS NOT TO BE USED FOR ANY PURPOSES. GE HEALTHCARE EQUIPMENT IS NOT TO BE USED FOR ANY PURPOSES. GE HEALTHCARE EQUIPMENT IS NOT TO BE USED FOR ANY PURPOSES. GE HEALTHCARE EQUIPMENT IS NOT TO BE USED FOR ANY PURPOSES.

GE Healthcare
 IS Services Design Center
 Milwaukee, Wisconsin